

IR Analysis Report

Instrument type Alpha
Accessory ATR platinum Diamond 1 Refl #9989BC2D
Operator Administrator
Spectrum file name PA6-Pellet.0
Measurement date and time 29/11/2010 16:30:39 (GMT+1)
Sample name PA 6.10 schwarz Pellets (3) | Av. of 3
Sample form ATR platinum Diamond 1 Refl (high pressure)


Quick Compare

Sample is identified ✓

Method file D:\Polymers.qcm (2014/08/19 16:14:19 (GMT+2))
Comment Polymer Identity
Threshold 95.00

Reference D:\Quick Compare Polymers\Polyamide 6 (PA 6).0 Correlation 96.50 % ■

Reference Spectra and Query Spectrum (red)

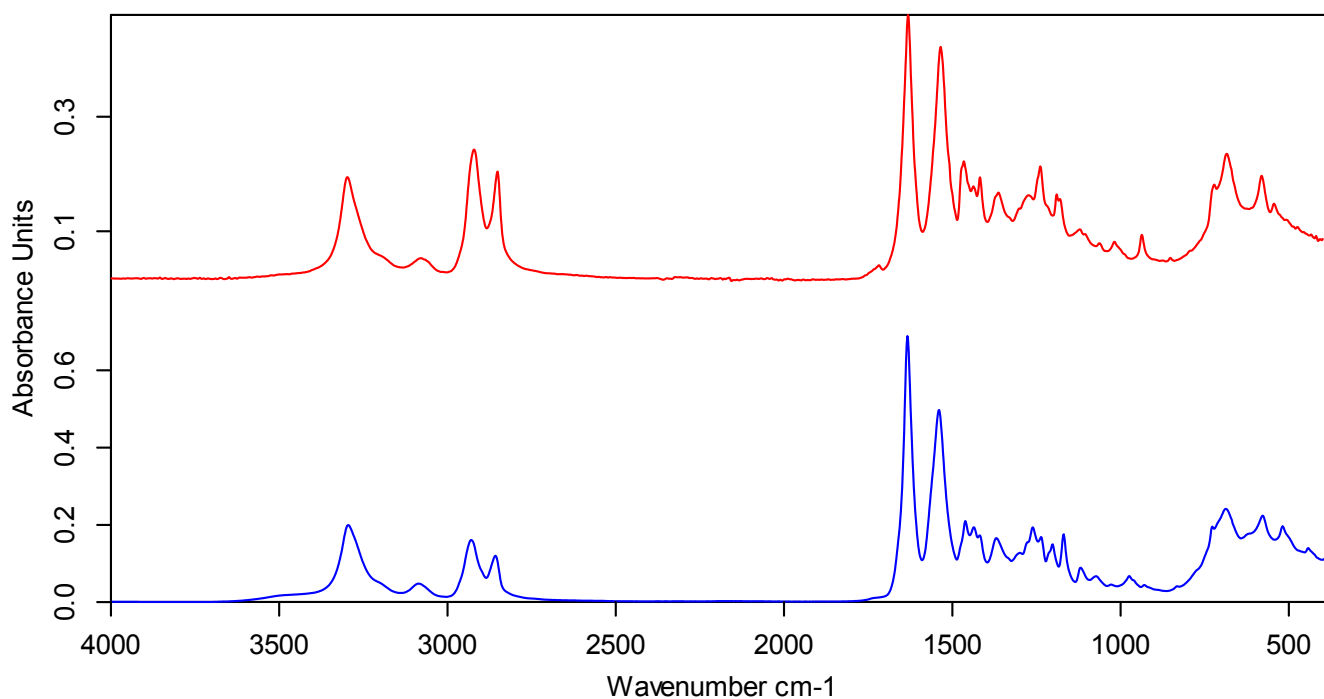

Signature 1

Signature 2